



TRUE LOCK Distal Radius Dorsal Anatomic Plates are indicated for;

- Dorsally displaced fractures
- Extra-articular fractures with metaphyseal defect (AO classification 23-A3)
- Open joint reconstruction (AO classification 23-C1, C2, C3).
- Combination of distal radius with carpal and metacarpal fractures.
- Corrective osteotomies.

Anatomical plate; right & left.


5 hole option between 3-7.

TRUE LOCK Distal Radius Dorsal Anatomic Plates are made of Ti6Al4V ELI material (ASTM F136).

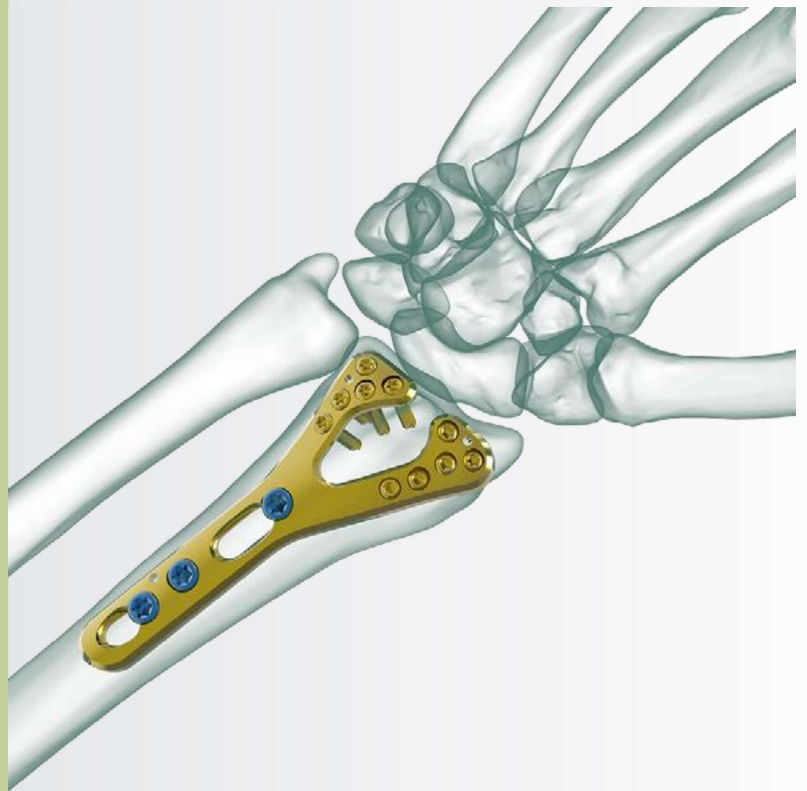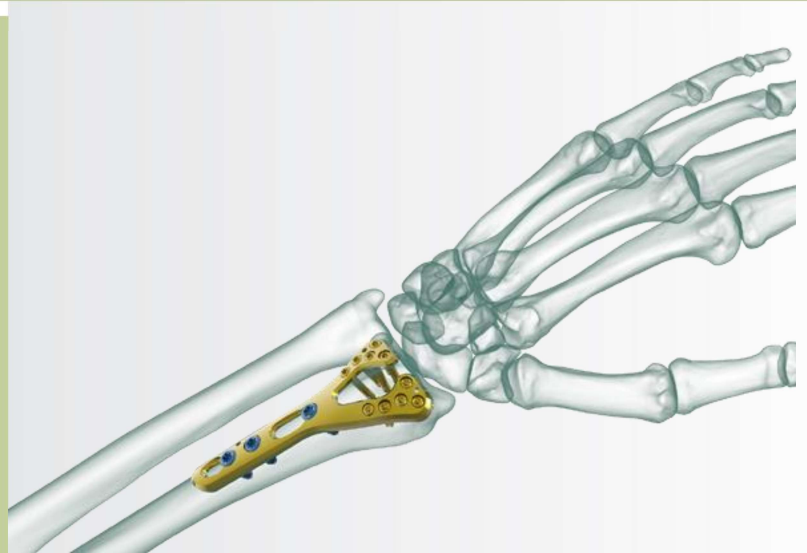


TRUE LOCK Distal Radius Dorsal Anatomic Plate Features

Elongated Combi holes in the neck and shaft facilitate plate adjustment and allow locking or compression options

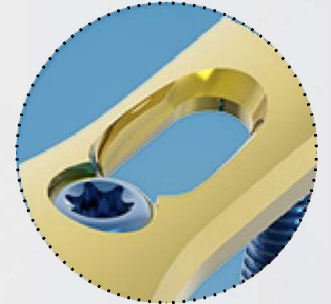


Low plate-and-screw profile and rounded plate edges minimize potential for tendon and soft tissue irritation

Kirschner wire holes accept Kirschner wires (up to 1.5 mm) to temporarily fix the plate to the radius to temporarily reduce articular fragments, and to confirm the location of the plate, relative to the radius.

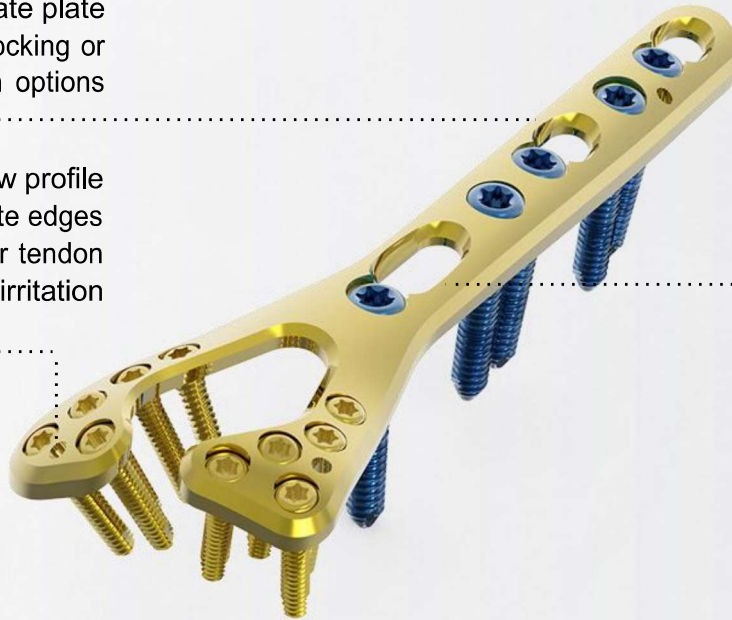

The combi-hole provides flexibility of axial compression and locking capability throughout the length of the plate shaft.

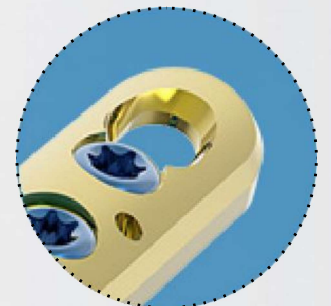

TRUE LOCK Distal Radius Dorsal Anatomic Plate Screws Info

Reference Number:	Hole Count:	Length (mm)
(L) 201-10191-003 (R) 201-10192-003	3 hole	70
(L) 201-10191-005 (R) 201-10192-005	5 hole	90
(L) 201-10191-007 (R) 201-10192-007	7 hole	105


2.3 mm Locking Cortical Screw




2.7 mm Non-Locking Cortical Screw



2.7 mm Locking Cortical Screw



3.5 mm Non-Locking Cortical Screw



3.5 mm Locking Cortical Screw

